

202240 DE 4800

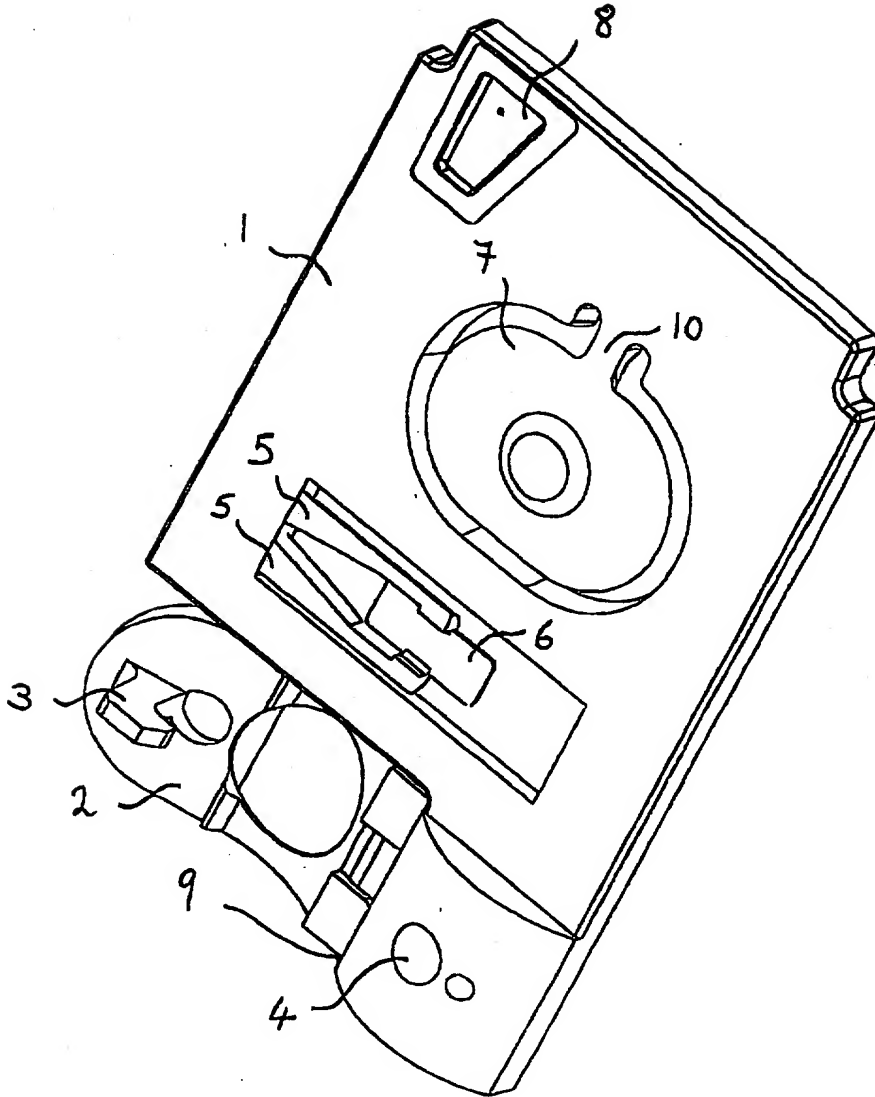


FIGURE 1

20240730.04202

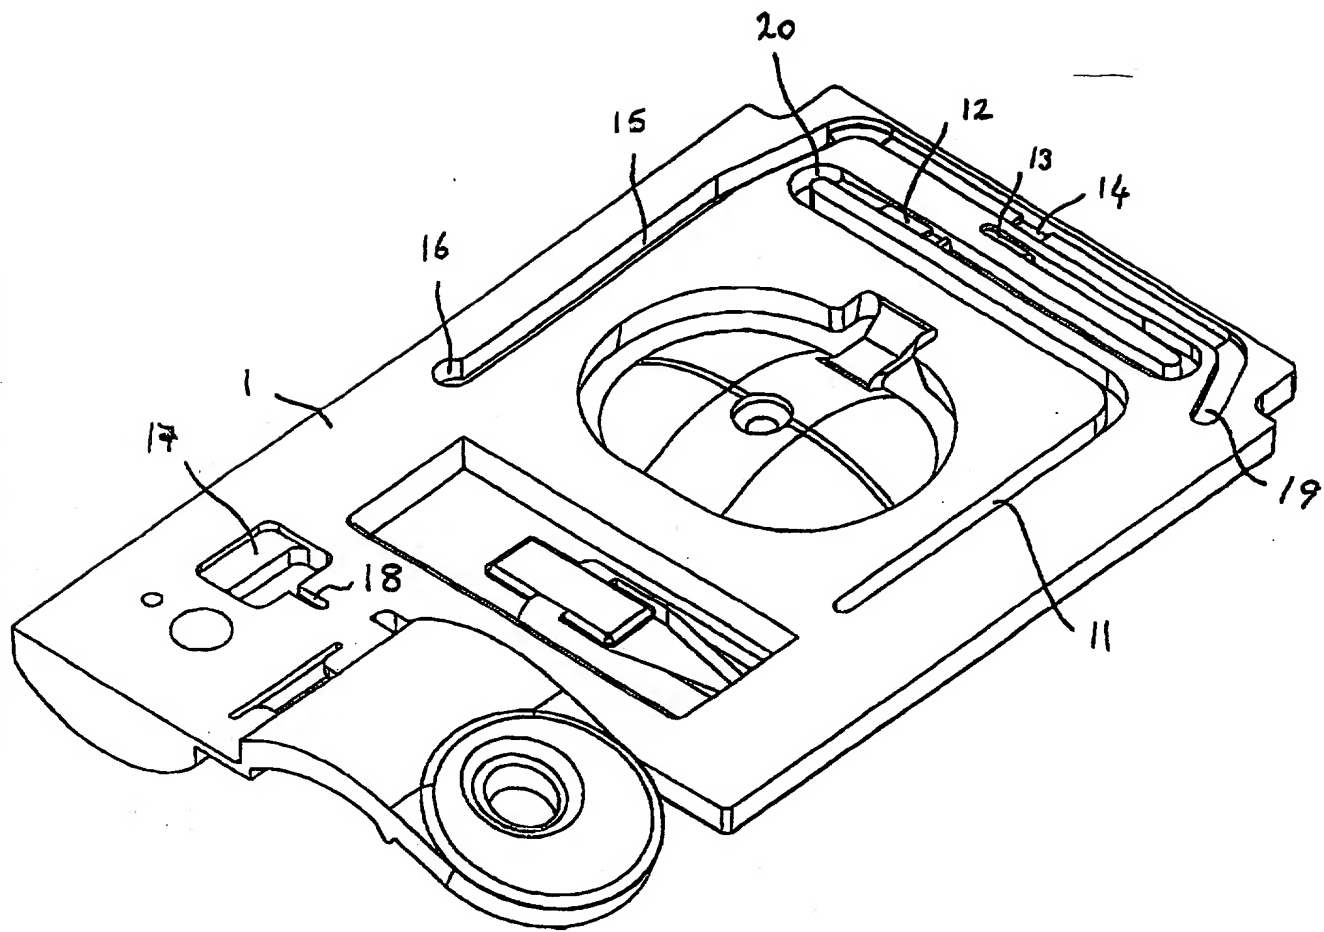


FIGURE 2

202240-032800T 1008730-04202

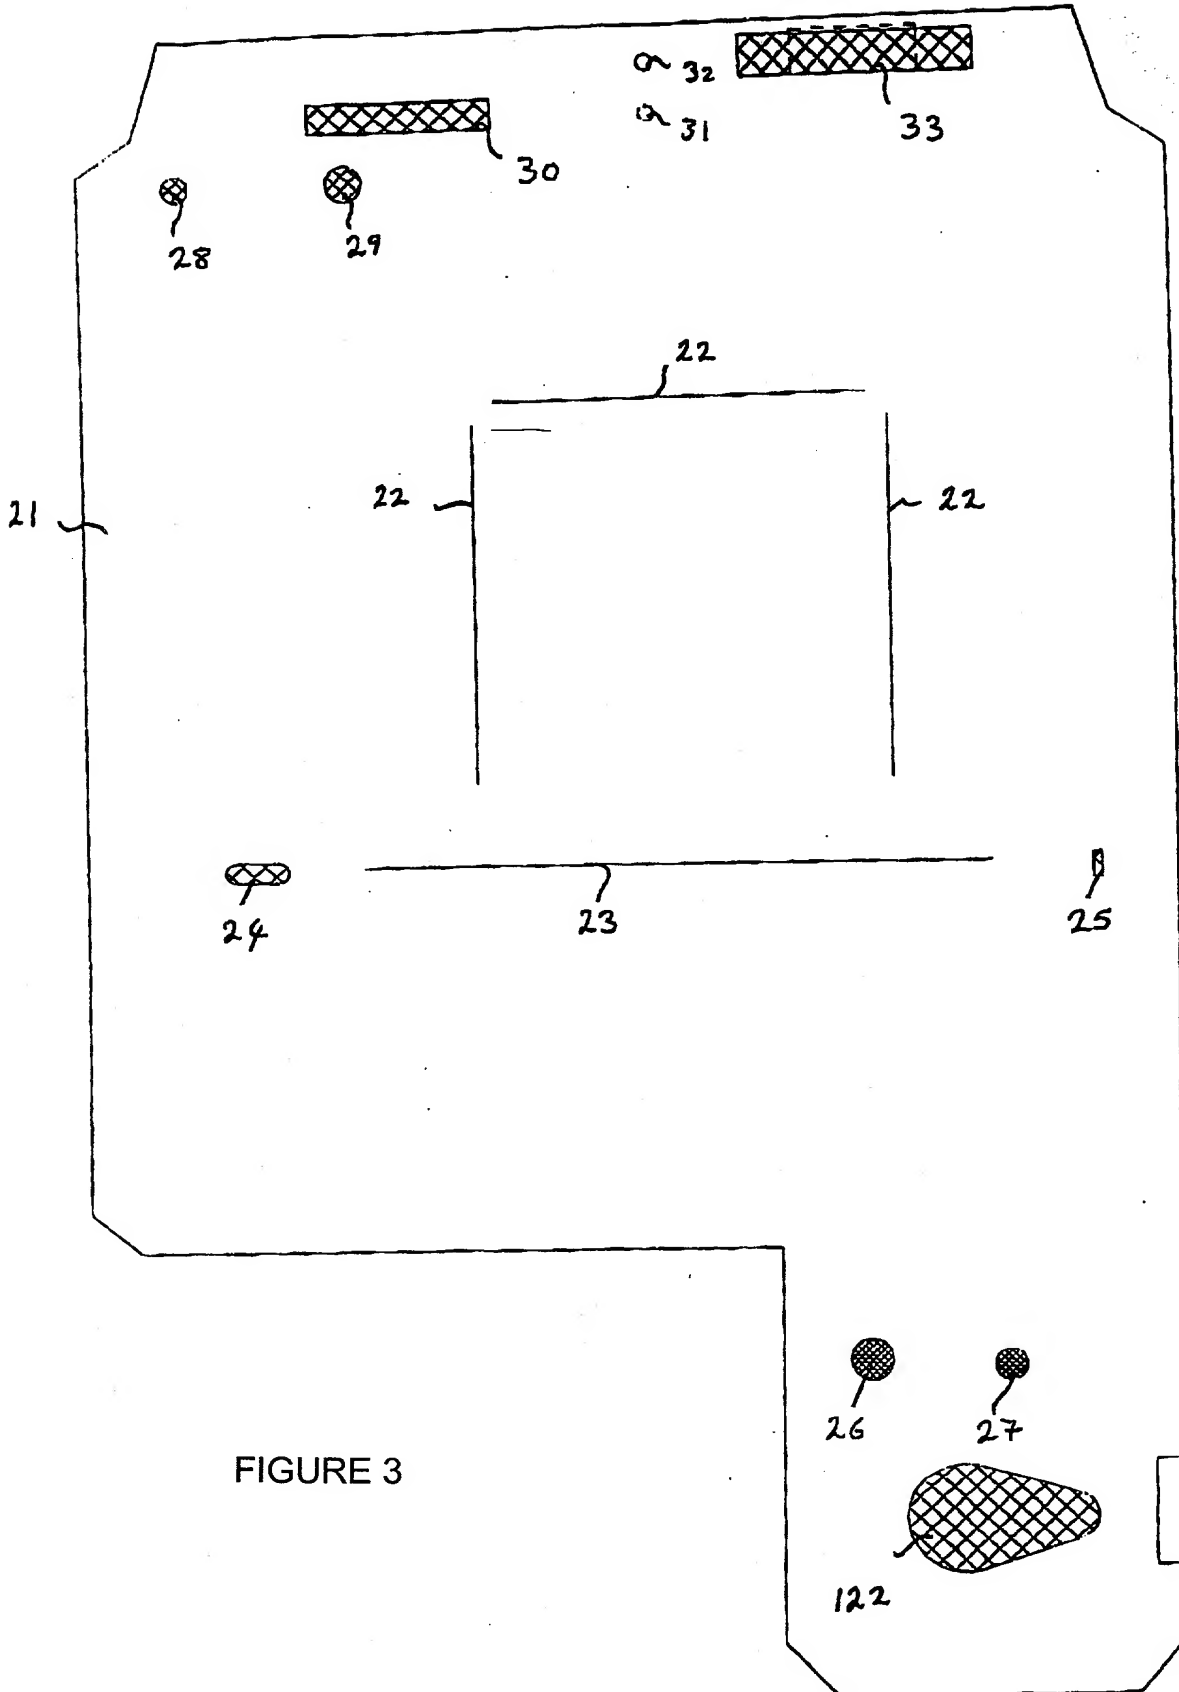


FIGURE 3

200240-083800T 10087730-042002

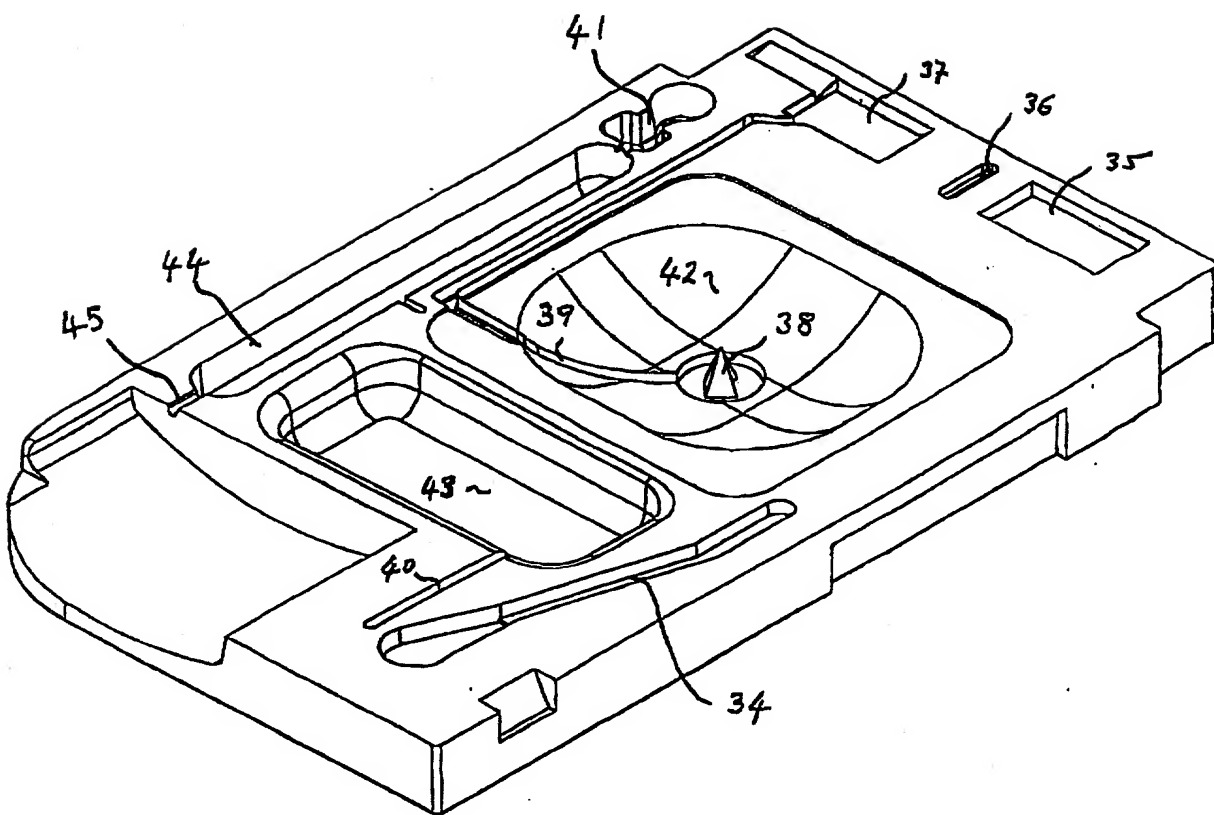


FIGURE 4

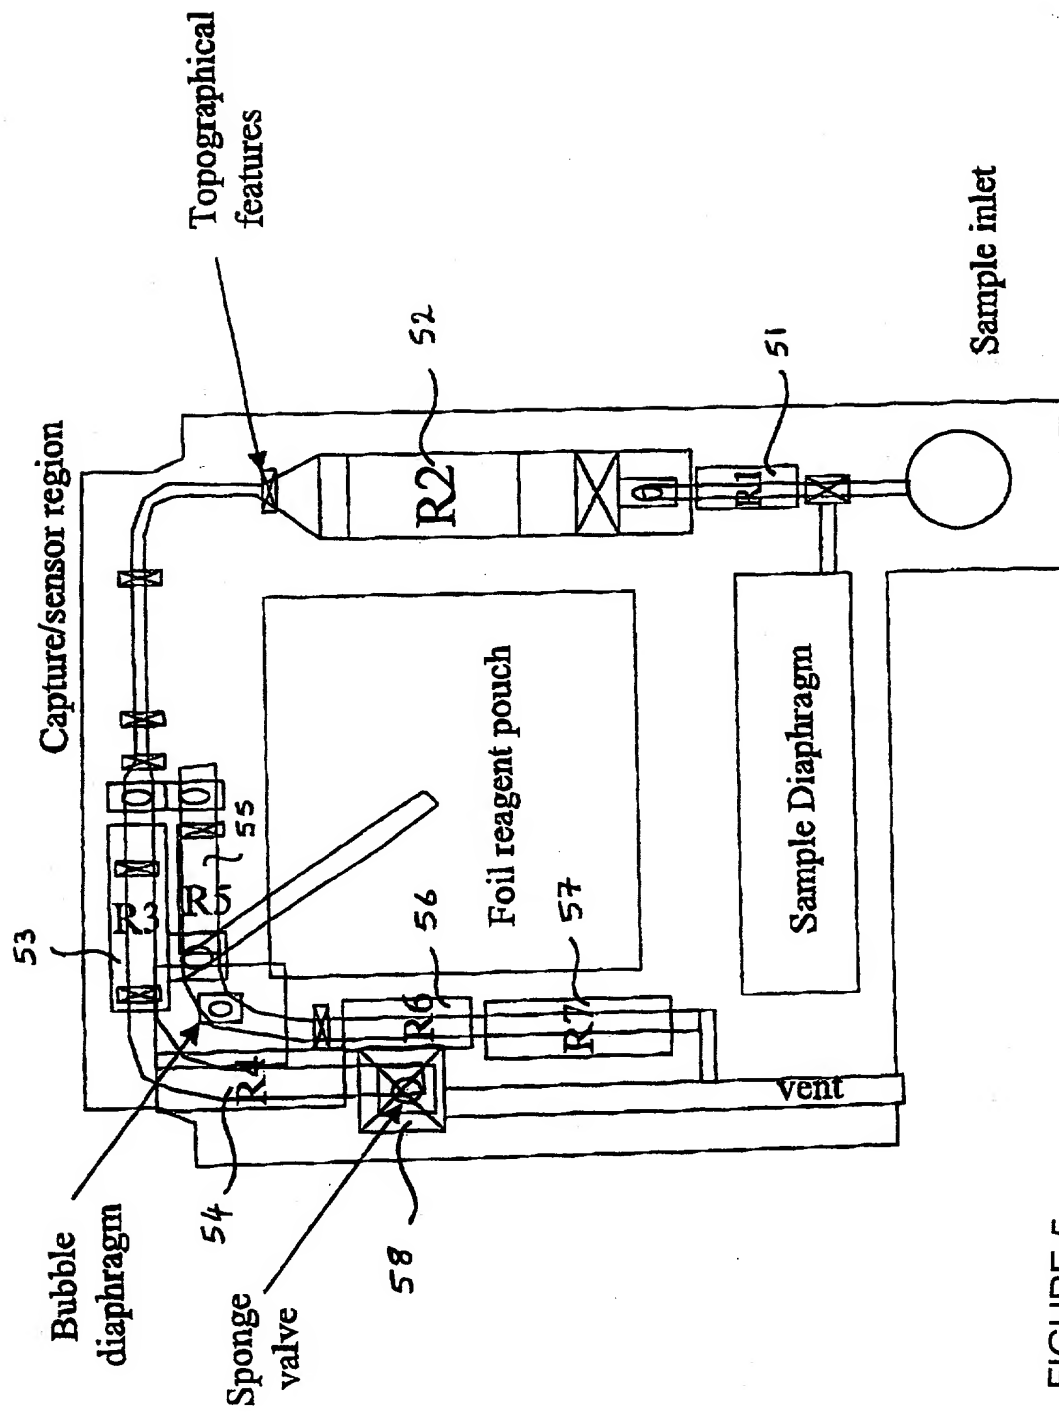


FIGURE 5



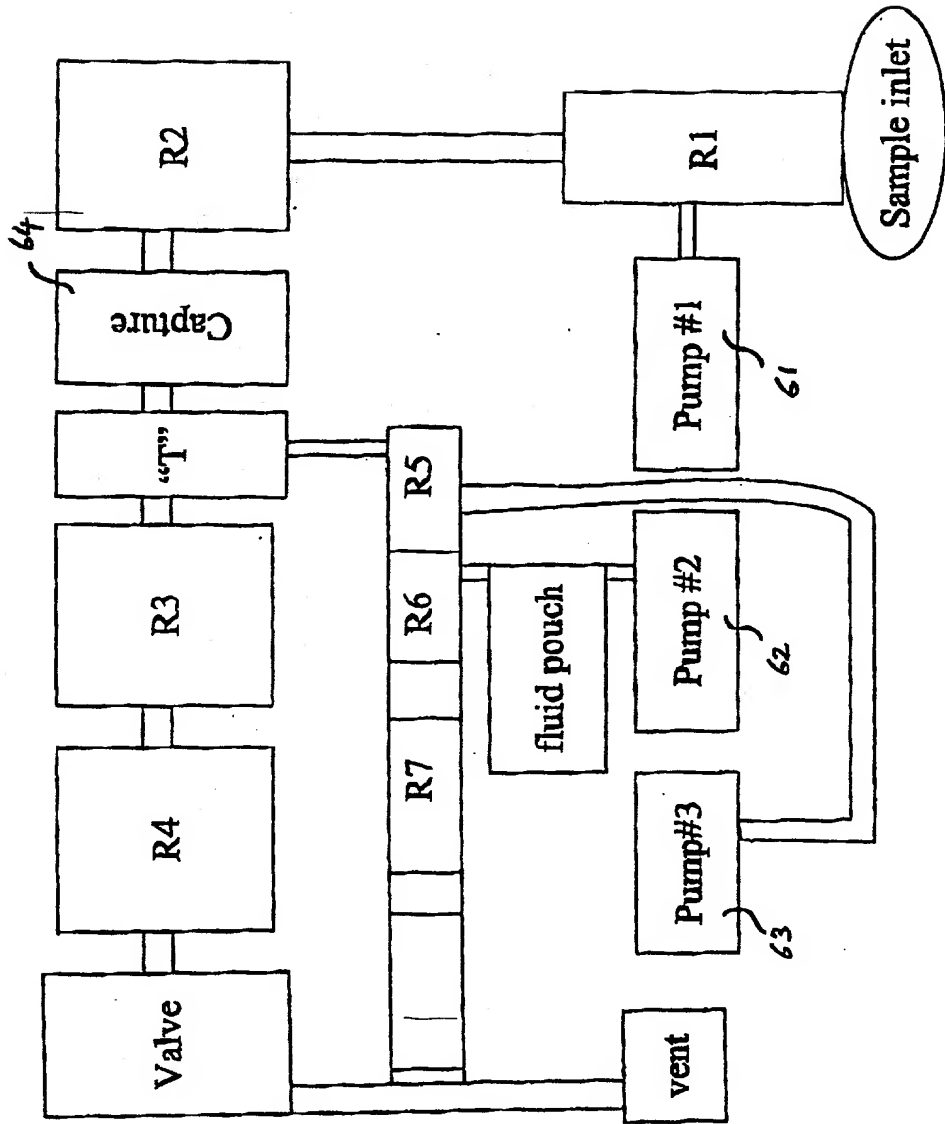


FIGURE 6

# Simultaneous Sandwich ELISA for Troponin I and other Cardiac Marker tests

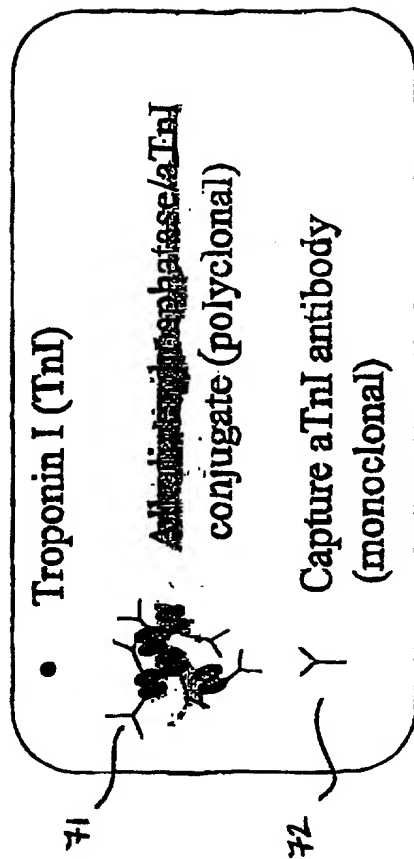

## 1: Capture Step

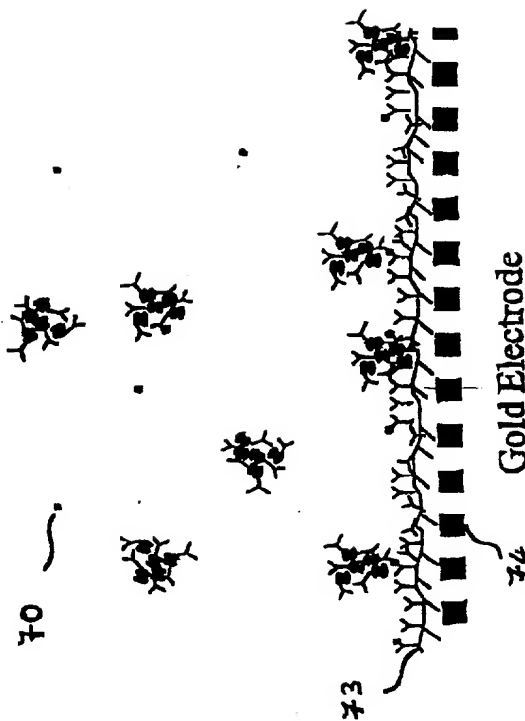

## 2: Wash and Analysis

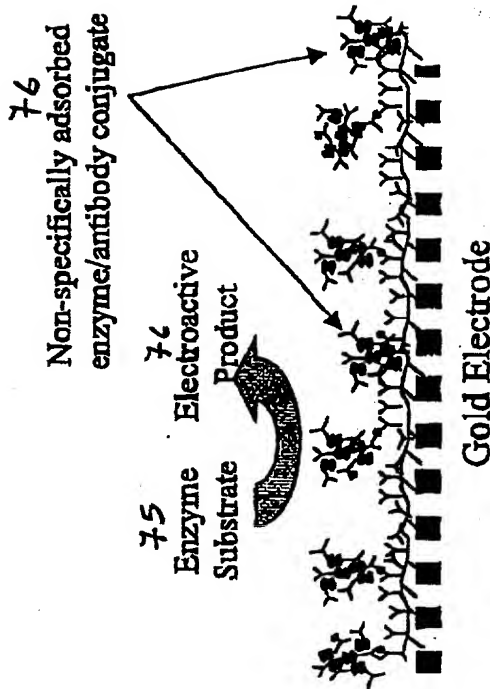


FIGURE 7

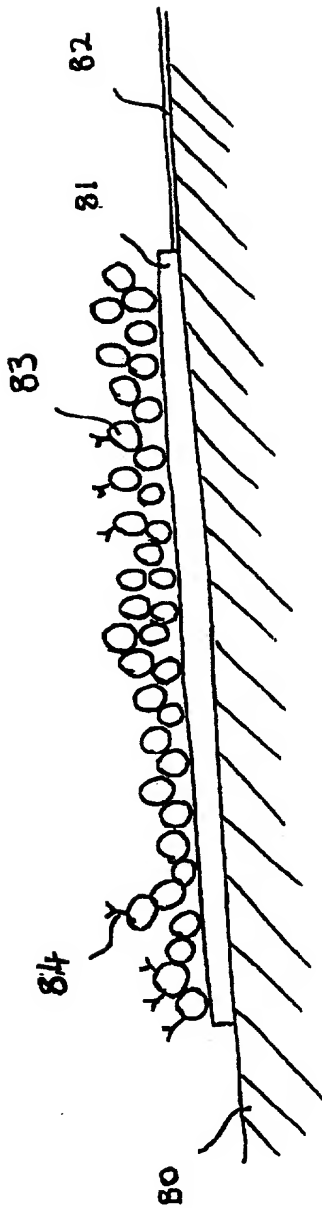


FIGURE 8



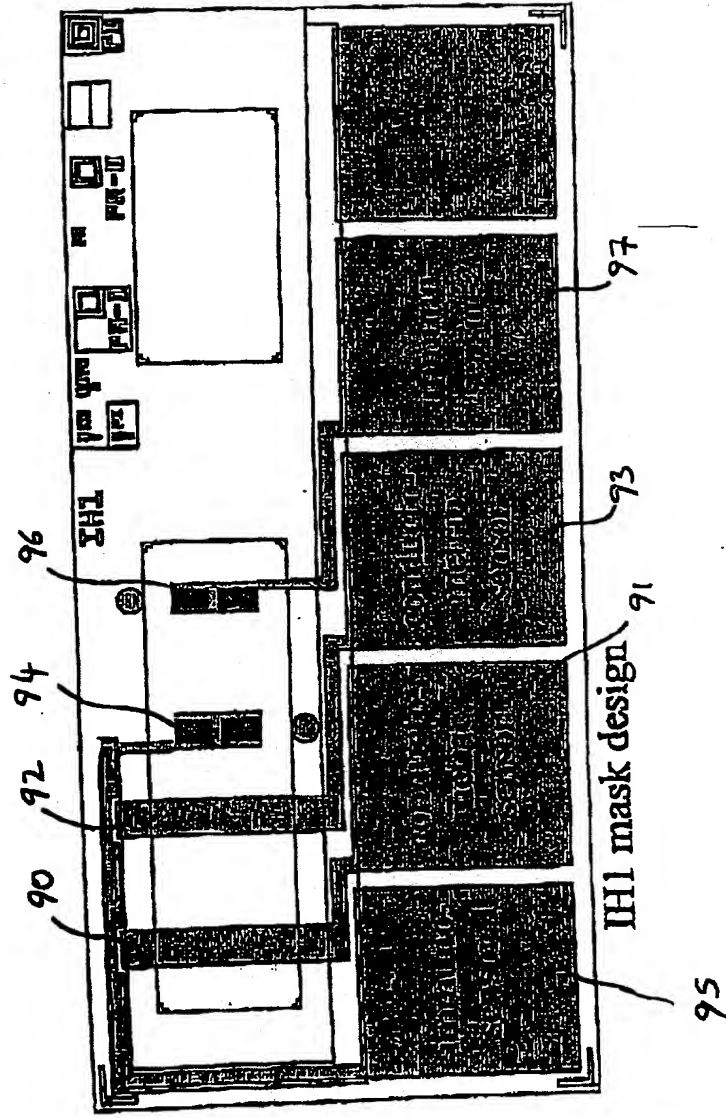


FIGURE 9

## 2 Level Precision (3 days, 2 sensor lots 8 analyzers)

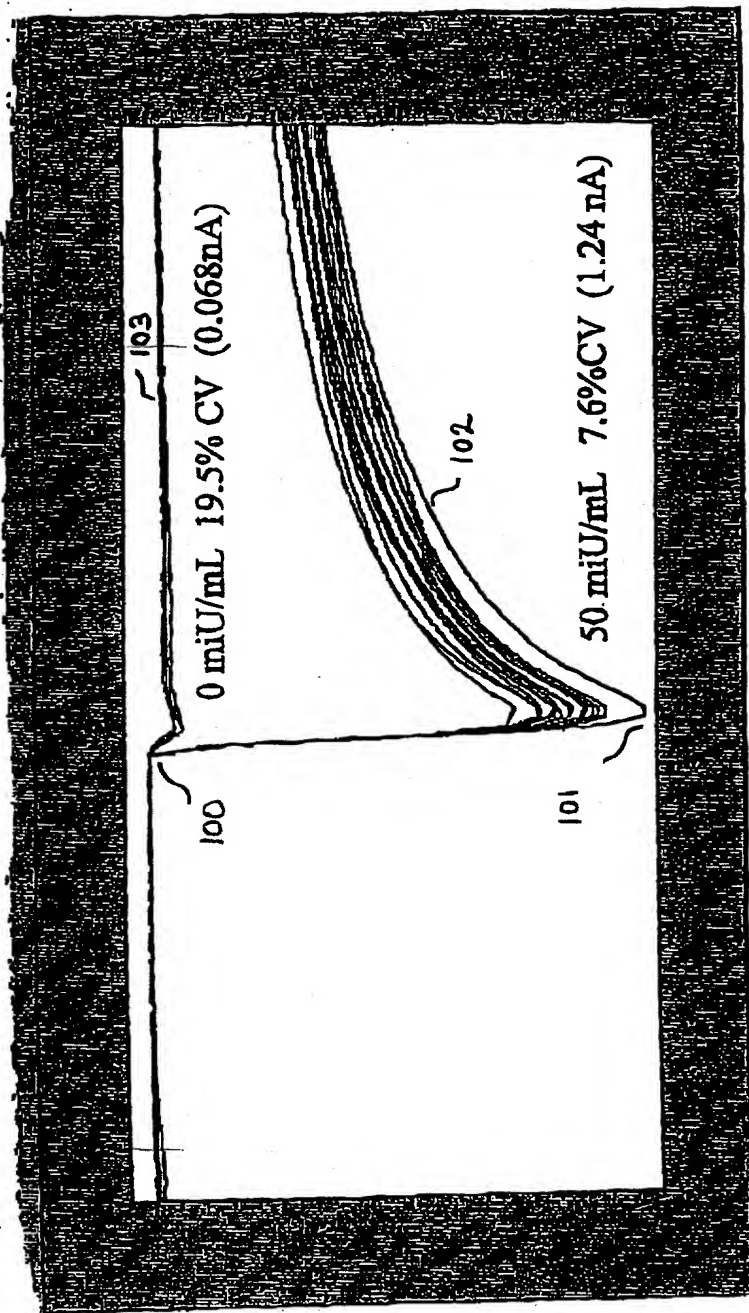


FIGURE 10

# IH-9 HCG Dose Response

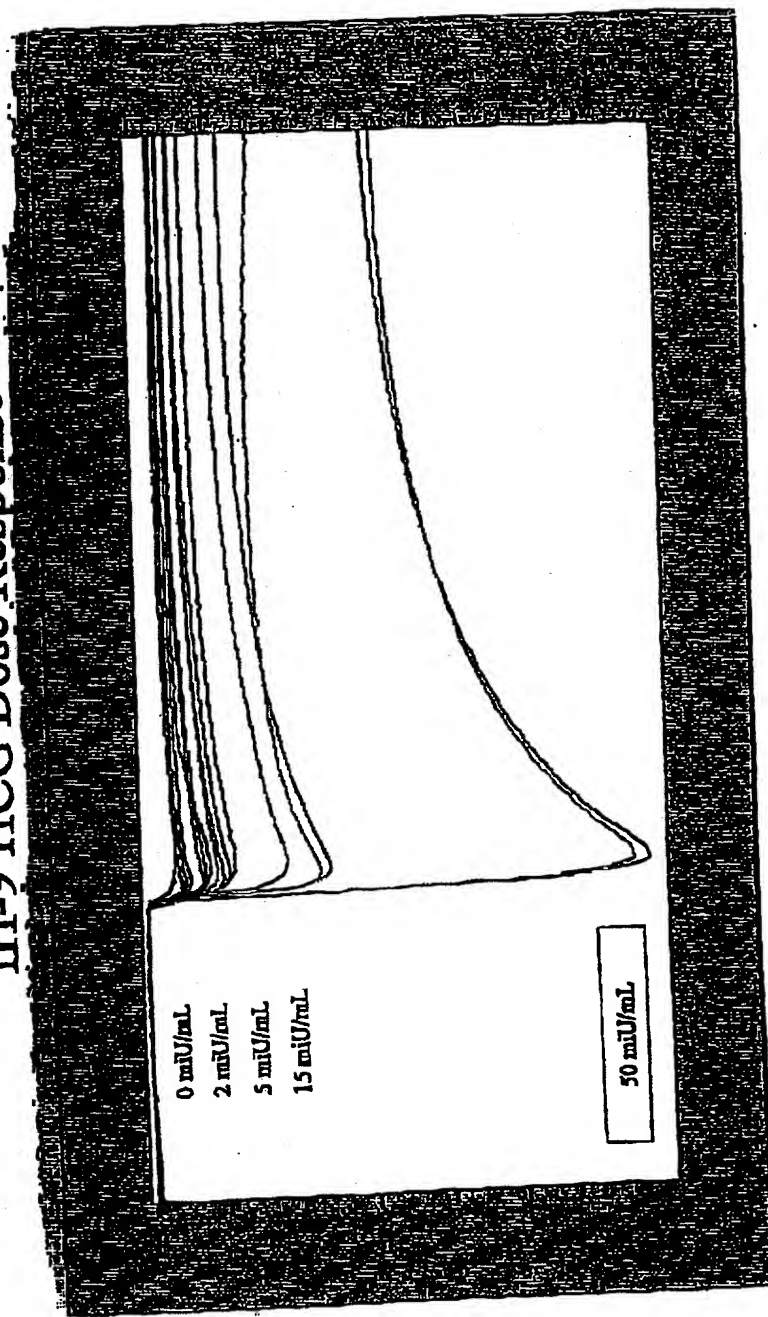


FIGURE 11

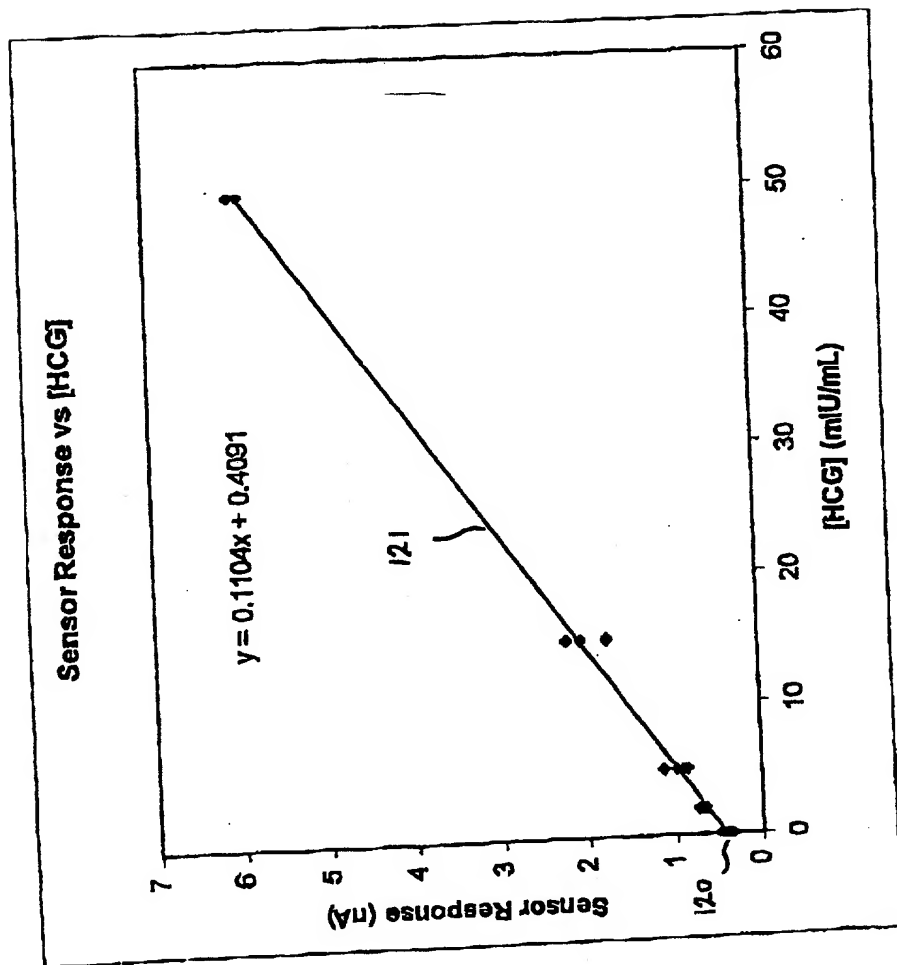


FIGURE 12

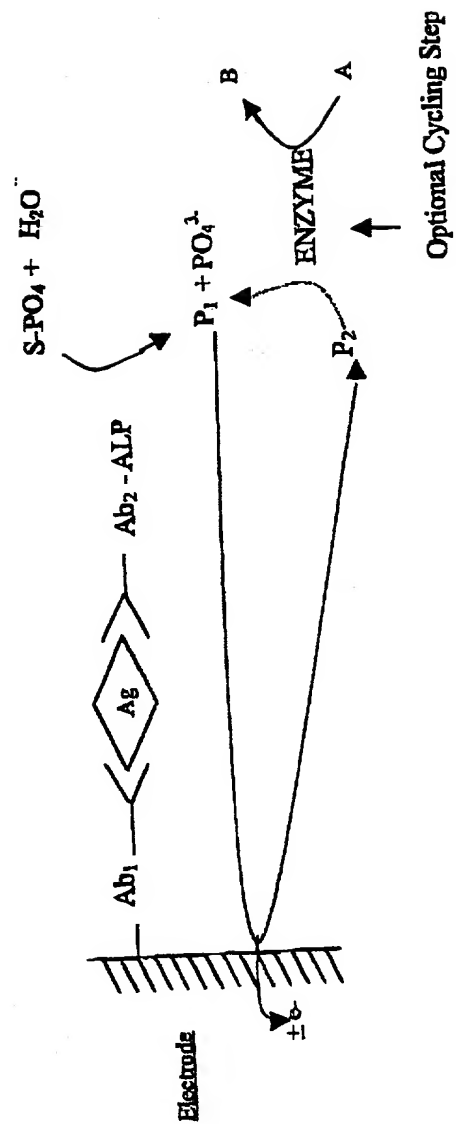


FIGURE 13

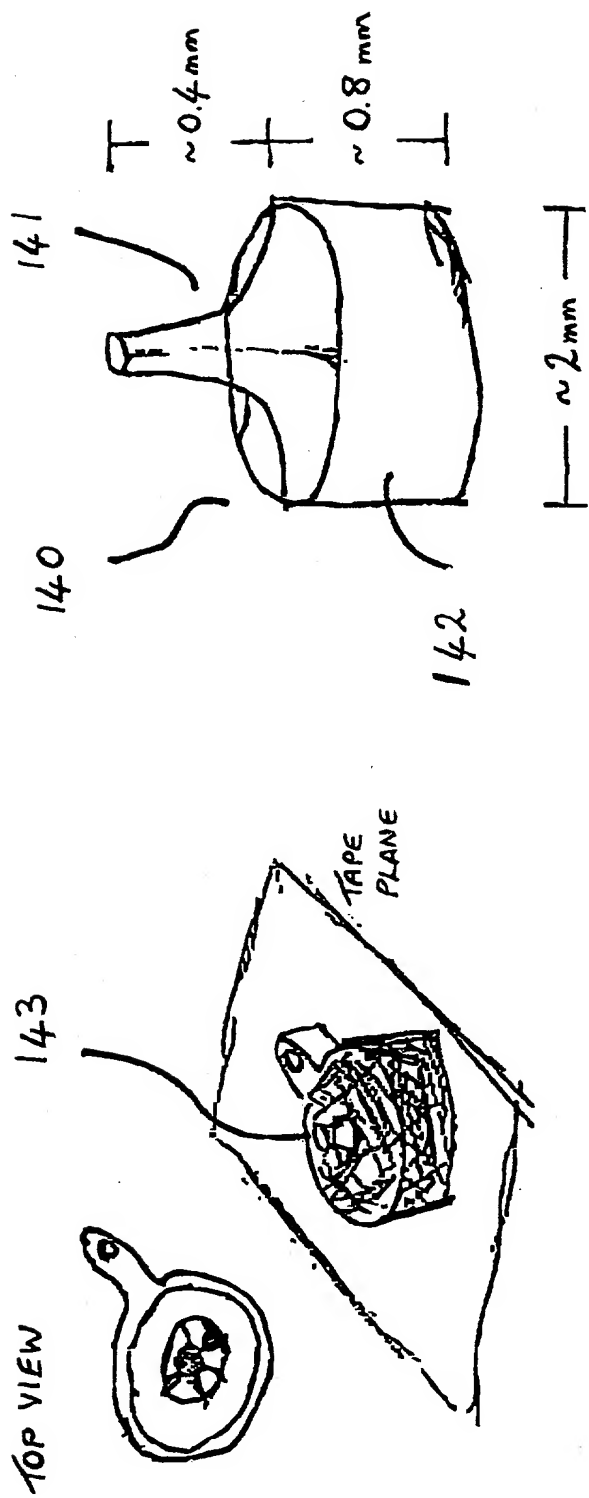


FIGURE 14

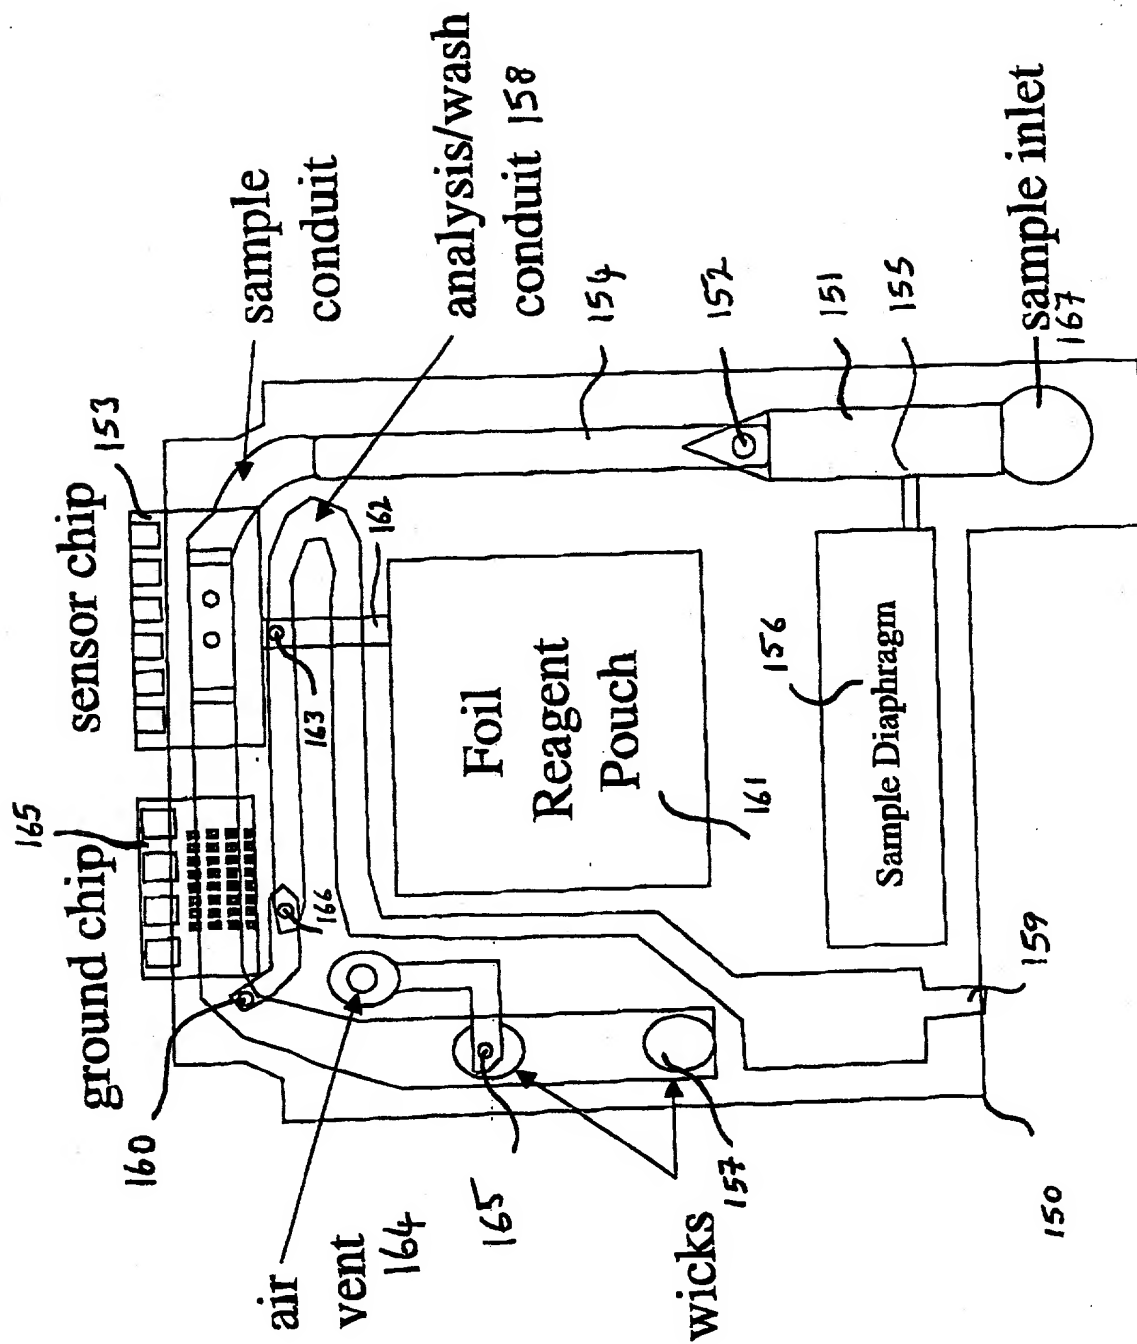


FIGURE 15

# Fluidic Schematic for i-STAT immunocartridge

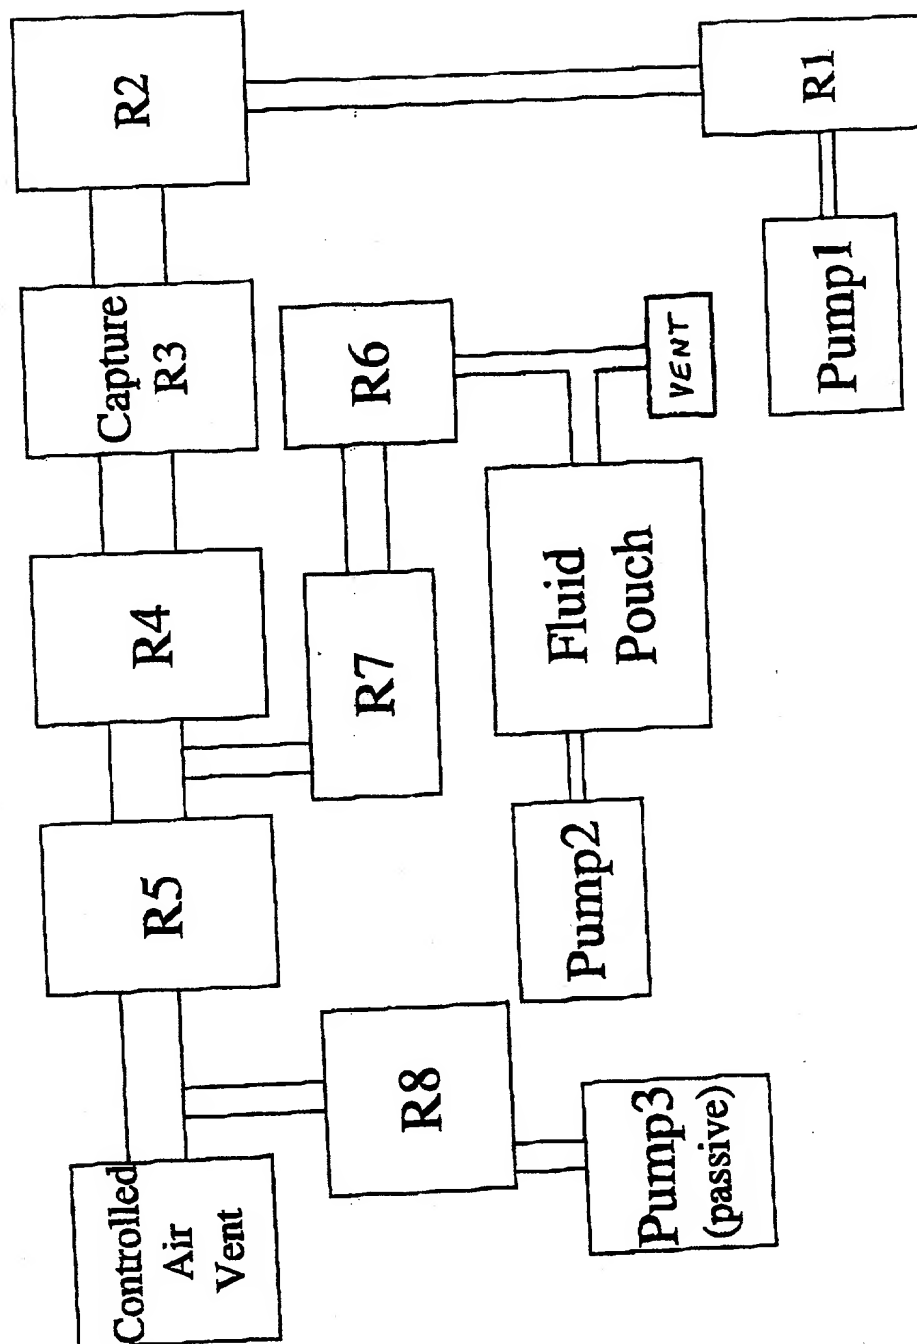


FIGURE 16



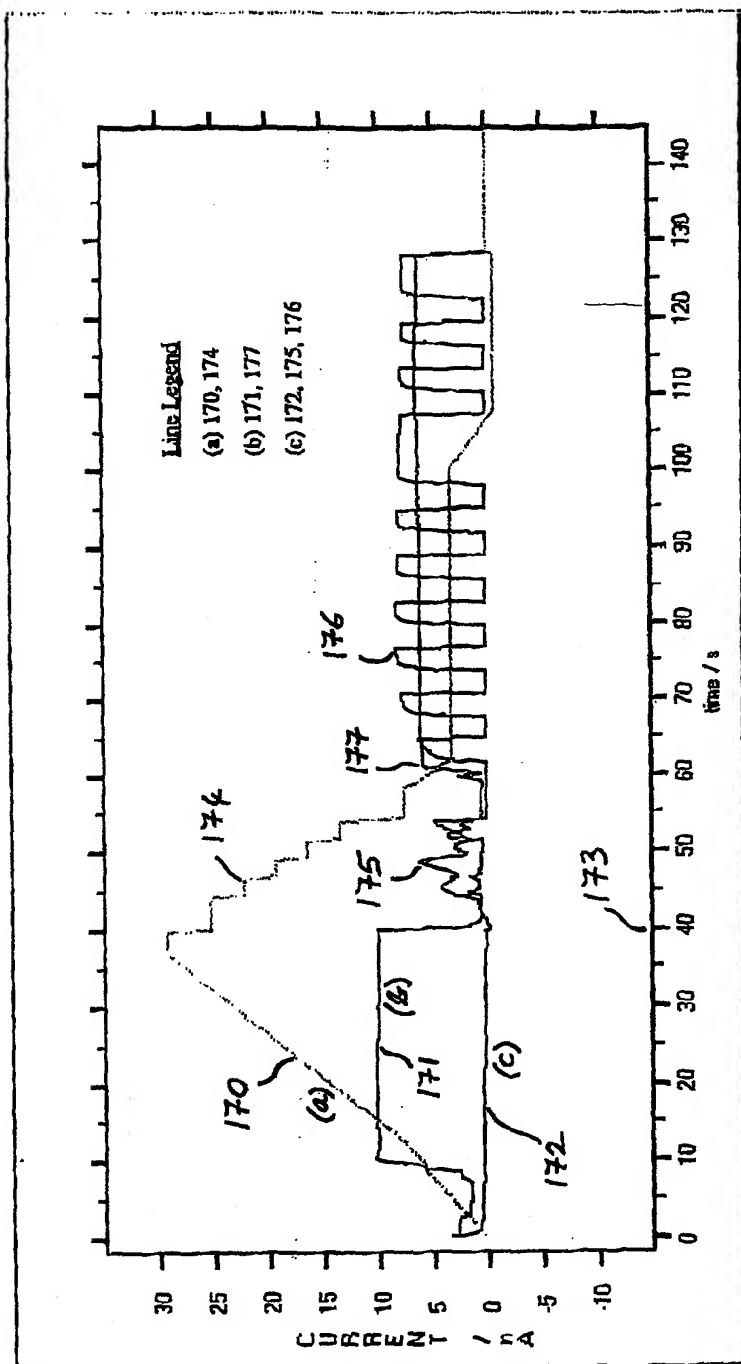


FIGURE 17